

Vessel Preparation of Femoropopliteal Lesions Prior to Drug-Coated Balloon Angioplasty with the



FLEX Dynamic Scoring Catheter


Nicolas Mouawad, MD - Chief and Medical Director, Vascular and Endovascular Surgery, McLaren Bay Region
 Richard Kovach, MD - Deborah Heart and Lung Center
 Daniel Leung, MD - Christiana Care Health Services

Purpose

Vessel preparation (VP) prior to the implementation of drug-coated-balloons (DCB) is increasing in clinical importance. VP has the potential to improve acute results of DCB by decreasing dissections and limiting stenting. VP should also provide an optimal environment for drug-uptake potentially leading to improved long-term outcomes.

Methods

FLEX Dynamic Scoring Catheter, a non-balloon-based scoring device, was studied as a VP device prior to DCB. Retrospective review of 263 real-world cases (50 institutes, 74 physicians) was performed.

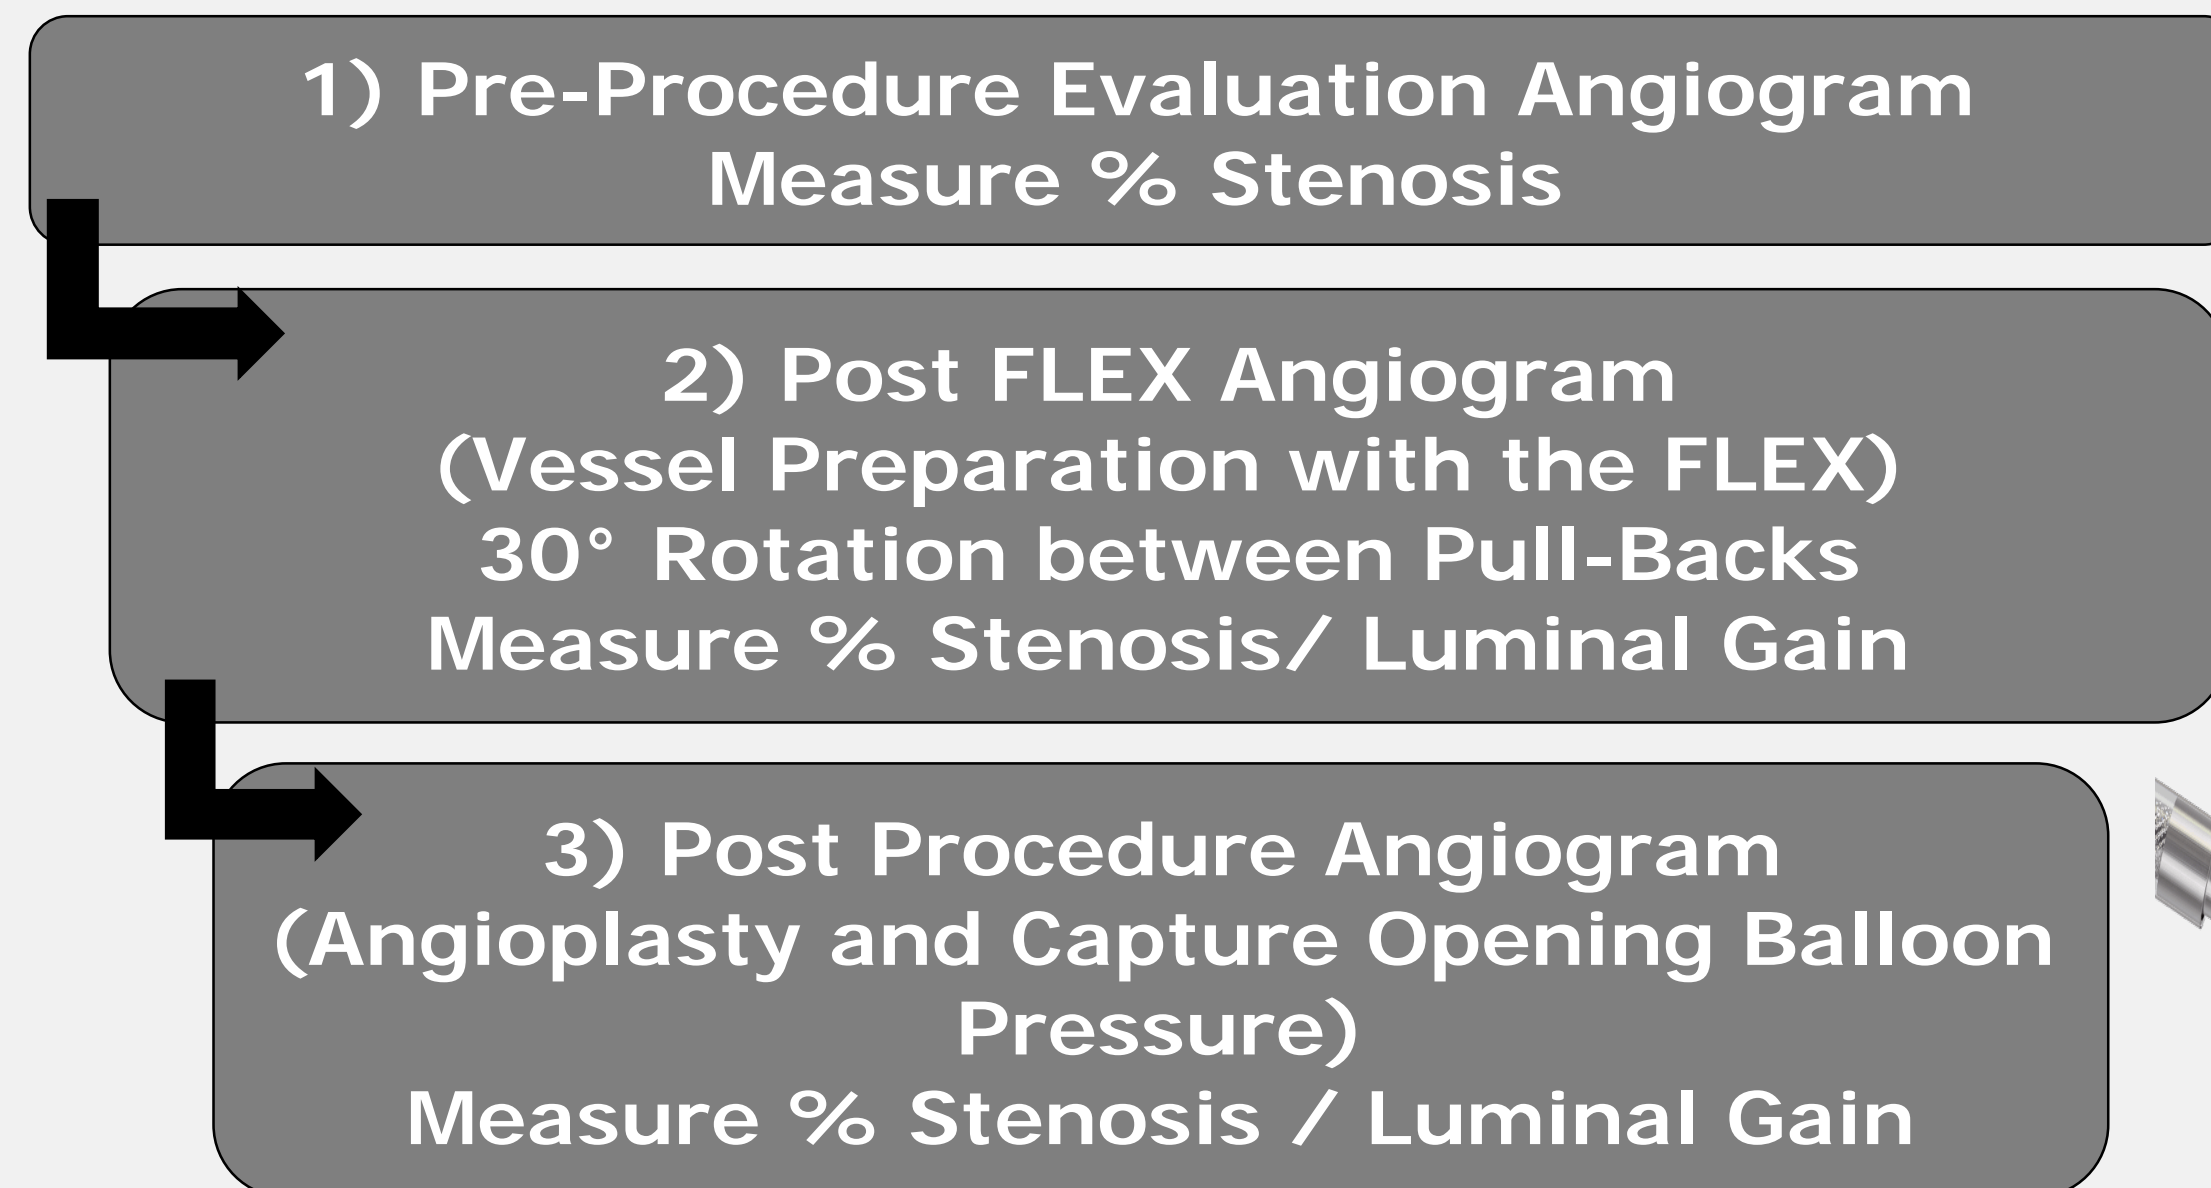

Pre-dilation using plain-old-balloon-angioplasty (POBA) was performed at the discretion of the operator. Dissection, luminal gain, and opening balloon pressures (lowest pressure required to fully efface the lesion) were the focus of this review.

Vessel Characteristics

Average Lesion Length	135 mm (2-410 mm)
Average Vessel Diameter	5.5 mm (2-8 mm)
Average Baseline Stenosis	91.7% (50-100%)
% CTO	45%



Results

Post FLEX	
Average Number of FLEX Passes	4
Residual Stenosis	65.3%
Luminal Gain	26.6%
Adjunctive Therapy with DCB	
Average Opening Pressure	4.4 atm (2-12 atm)
Maximum Pressure	9 atm (3-15 atm)
Residual Stenosis	9.3% (0-40%)
Procedural Complications	
Grade A Dissections	1%
Grade B Dissections	4%

Bail-out stenting was not required.
No flow-limiting dissections, perforations, or emboli occurred.


Technology Overview

One-Size-Fits-All Device / 1 SKU Inventory
 6 Fr / .014 and .018 Guidewire Compatible
 40 cm and 120 cm Working Length
 Engineered for continuous parallel micro-incisions by 3 Atherotomes
 FLEX predilates the stenosis → Skids apply a constant pressure (1 atm)
Controlled depth micro-incisions (Atherotome Height 0.01")
 Rotationally controlled, provides the ability to create multiple scores

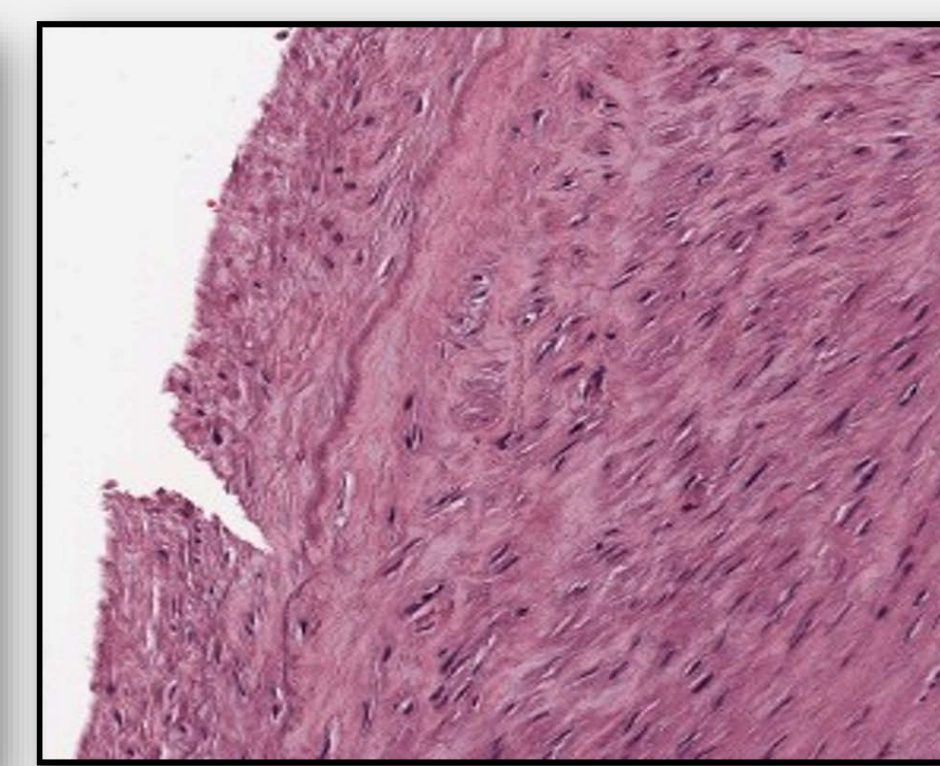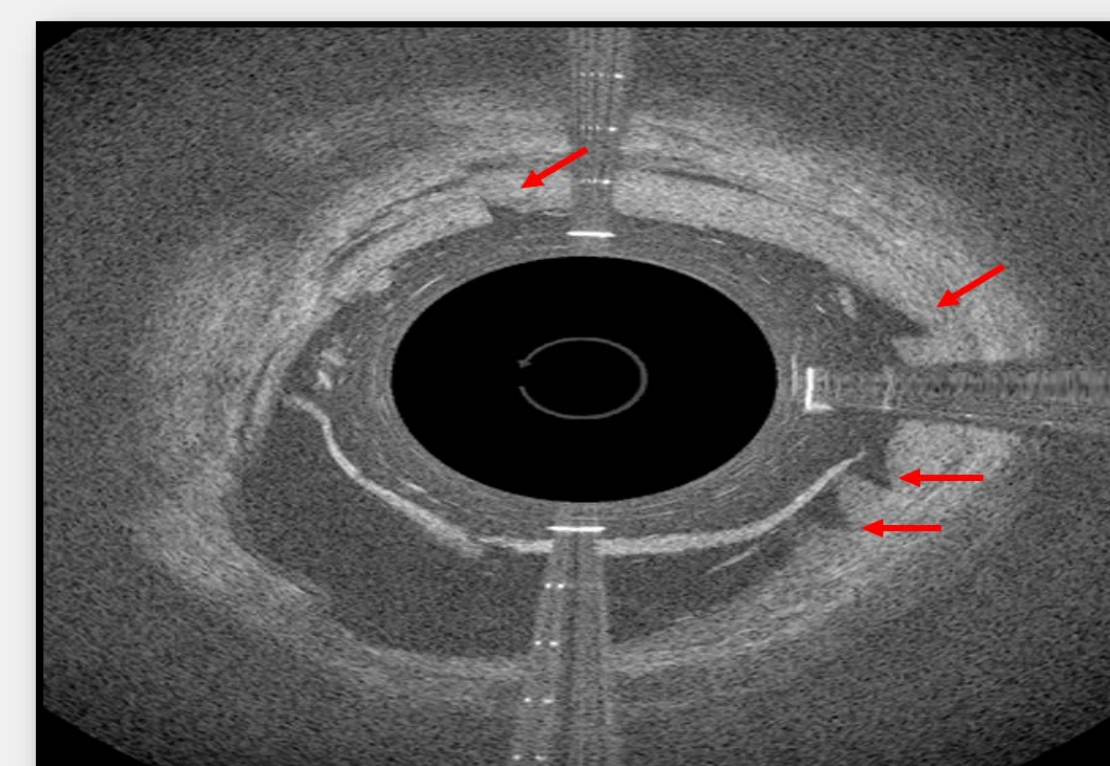


OCT Image (left) and Histology (right) of a Human Cadaver SFA FLEX Micro-Incision

Case Study

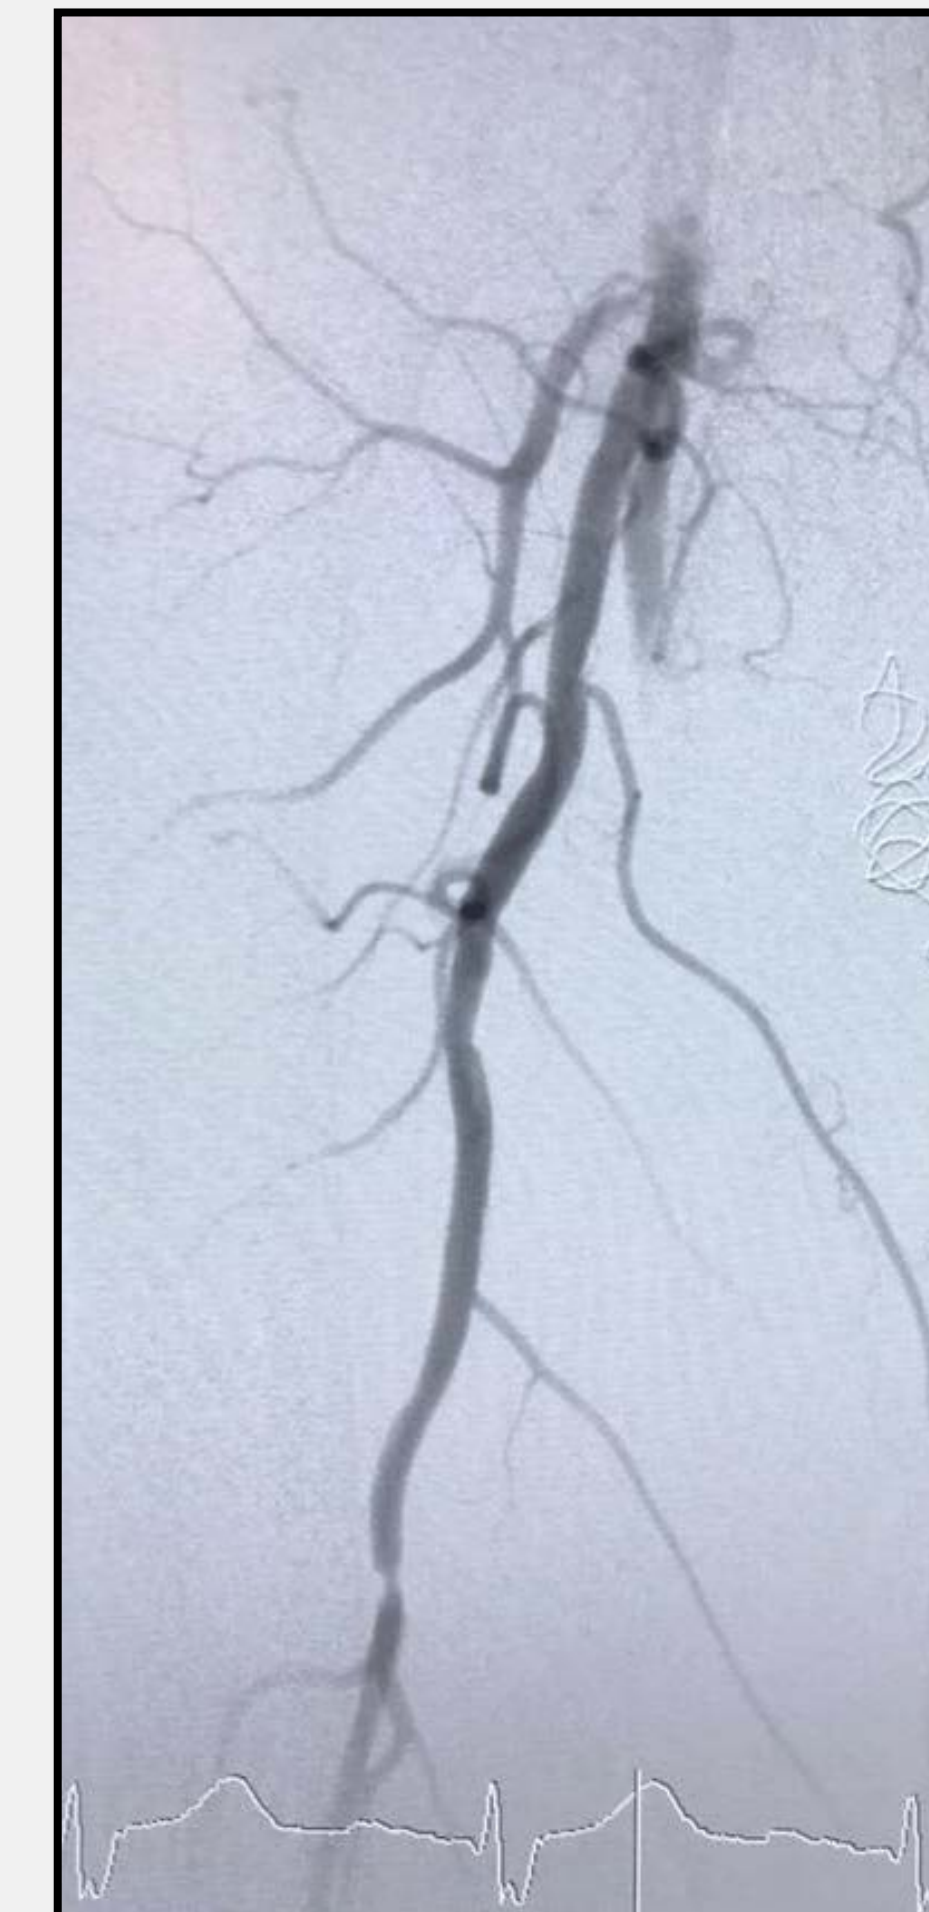

Vessel Diameter: 5 mm
 Lesion Length: 250 mm
 Calcification: Severe
 Pre Stenosis: 100%

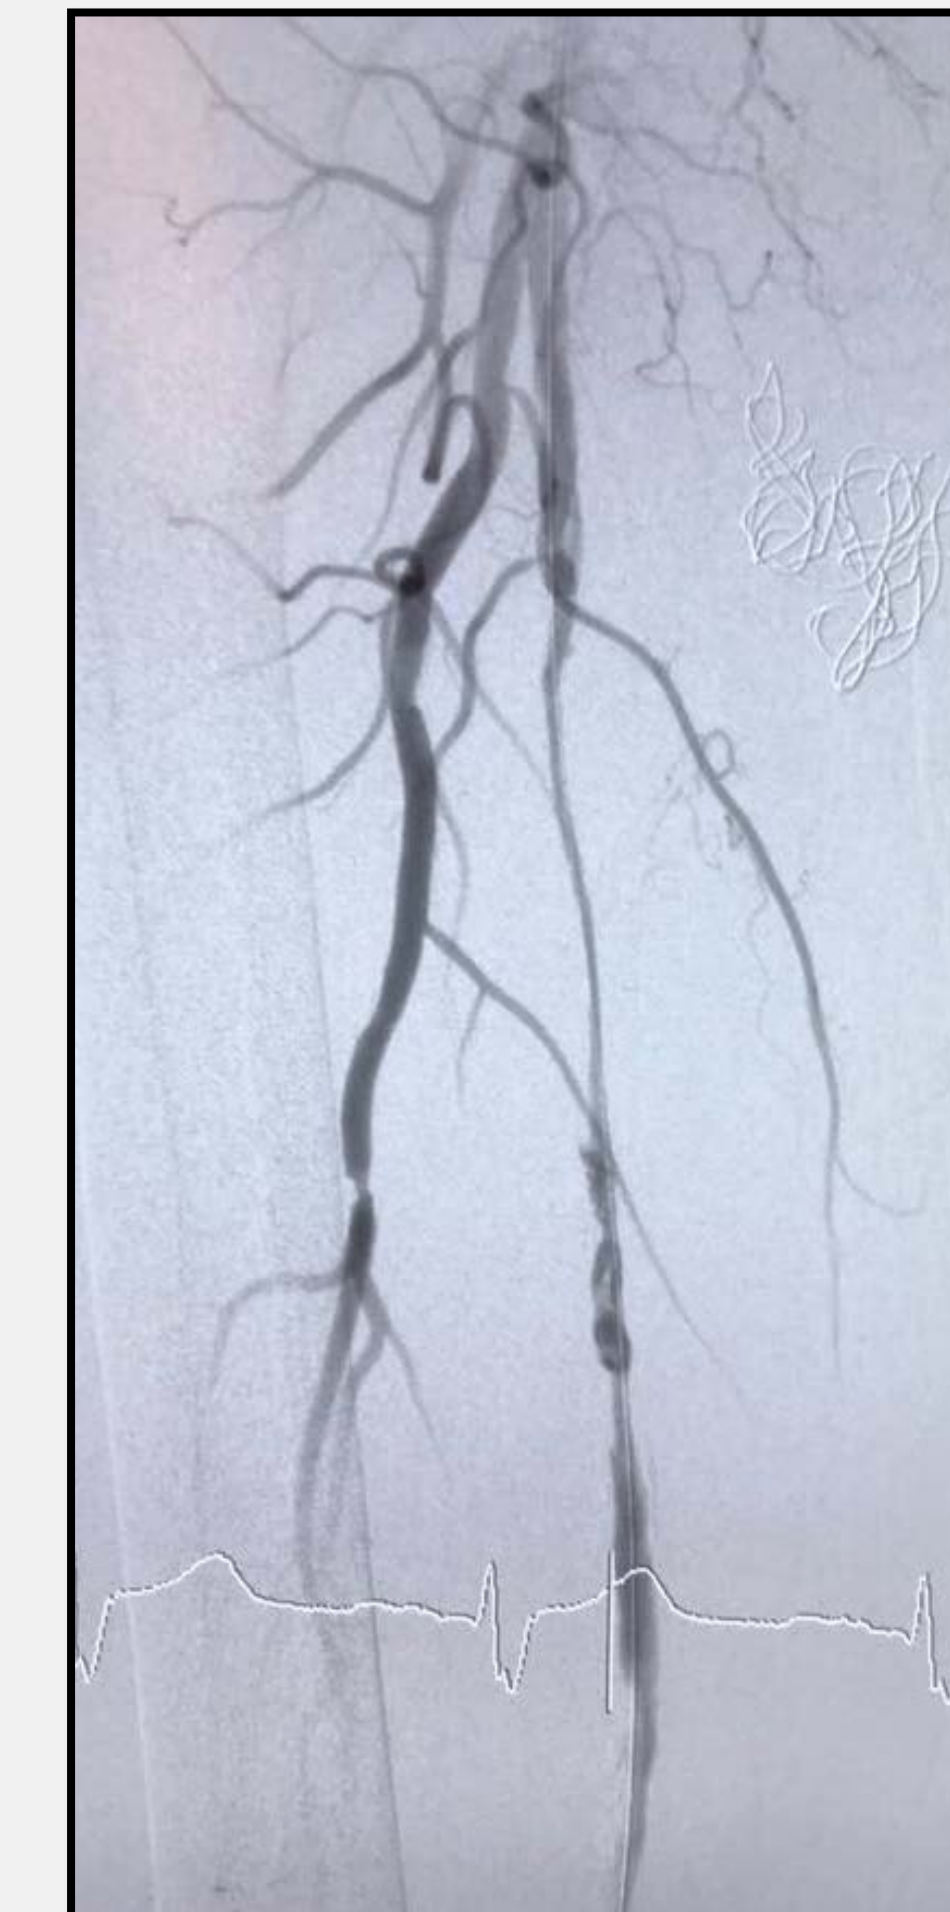

Post FLEX Recanalization
 3 FLEX Passes
 Post FLEX Alone
 Luminal Gain: 30%



Final Result
 Treated with a DCB
 Inflation Time: 3 min
 DCB Opening Pressure: 5 atm
 Residual Stenosis: 5%

Conclusion

FLEX Dynamic Scoring Catheter is utilized by interventionalists as VP prior to DCB. A significant luminal gain was achieved. Observed adequate vessel compliance measured by low balloon opening pressures. Low rates of dissection were observed, suggesting VP can optimize results compared to angioplasty alone. Further studies are warranted to determine longer-term outcomes and demonstration of improving drug-uptake.